

# 64 Channel ASIC for Neurobiology Experiments

Paweł Gryboś, Piotr Kmon, Robert Szczygieł, and Mirosław Żołądź

**Abstract**—This paper presents the design and measurements of 64 channel Application Specific Integrated Circuits (ASIC) for recording signals in neurobiology experiments. The ASIC is designed in 180 nm technology and operates with  $\pm 0.9$  V supply voltage. Single readout channel is built of AC coupling circuit at the input and two amplifier stages. In order to reduce the number of output lines, the 64 analogue signals from readout channels are multiplexed to a single output by an analogue multiplexer. The gain of the single channel can be set either to 350 V/V or 700 V/V. The low and the high cut-off frequencies can be tuned in  $9 \div 90$  Hz and in the  $1.6 \div 24$  kHz range respectively. The input referred noise is  $7 \mu\text{V}$  rms in the bandwidth 90 Hz - 1.6 kHz and  $9 \mu\text{V}$  rms in the bandwidth 9 Hz - 24 kHz. The single channel consumes 200  $\mu\text{W}$  of power and this together with other parameters make the chip suitable for recording neurobiology signals.

**Keywords**—Low noise amplifier, neural recording, ASIC, multichannel systems, neurobiology experiments.

## I. INTRODUCTION

ACCESSIBILITY of modern semiconductor technologies makes it possible to produce electronic multichannel systems consuming low power and occupying small area. Also biotechnology has made a large progress and offers biocompatible multichannel electrodes for neurobiology experiments. Thus in the last decade there is a rapid growth of projects [1] which aim to build measurement systems able to record neurobiological signals from many neurons at the same time. All of these researches are conducted since people like to delve into nervous system in order to understand how it works. This knowledge can be then very helpful in building artificial prosthesis for disabled persons, in finding cures for diseases such as Parkinson or Alzheimer or in reusing it for coding the large amount of information [2], [3].

The main obstacle with such applications is a need to collect the information from many (hundreds or even more) neurons simultaneously what leads to multichannel architectures of recording system. Thus one has to consider an application containing dozens of identical recording channels which main requirements are:

- low power consumption of the single channel (less than 500  $\mu\text{W}$ ) in order to preserve the tested tissue from overheating [4] and also to ensure long term recording in the case of using battery power supply,
- small area occupied by the entire electronic chip in order to build light recording system essential for in vivo experiments,

This research and development project was supported by Polish Ministry of Science and Higher Education in the years 2008 - 2010.

P. Gryboś, P. Kmon, R. Szczygieł, and M. Żołądź are with the Department of Measurement and Instrumentation, AGH University of Science and Technology, Krakow, Poland (e-mails: pgrybos@agh.edu.pl, kmon@agh.edu.pl, robert.szczygieł@agh.edu.pl, zoladz@agh.edu.pl).

- good uniformity of the main chip parameters such as corner frequencies of the recording channel, its gain and input referred noise,
- low input referred noise in order to record small input signals which amplitudes are from tens to hundreds of  $\mu\text{V}$ ,
- good functionality (the ideal would be the system able to record various neurobiology signals [5], so the one with possibility of changing its frequency band and gain, both in the wide range).

Despite all above requirements one has also to take into account other aspects of such systems. For instance, recording signals situated in a single Hz frequency band forces consideration of flicker noise  $1/f$  component which in modern VLSI technologies dominates in this frequency range. One has also to take into account large DC voltage offset which is generated at the electrode-tissue interface and can be large enough to saturate the input stage of recording amplifier. Additionally, the need of recording signals with very low frequencies (even below 1 Hz) obligates a designer to use filters with very large RC constants. This means that one has to employ high resistance structures which in modern technologies with limited silicon area is difficult to obtain.

The mentioned restrictions are sometimes mutually opposing (e.g. low input referred noise and low power consumption or good uniformity of the main parameters and small area occupied by the designed chip) which complicates a final chip and forces one to find optimized solutions.

Based on our experience in design and practical applications of such kind of ASICs for recording systems comprising of hundreds of electrodes [6], [7], [8] we propose a new 64-channel ASIC, which meets the above requirements.

The paper is organized as follows. Section II describes the ASIC architecture. The measurements are presented in the Section III and Section IV contains conclusions.

## II. CHIP ARCHITECTURE

In the Fig. 1 the microphotograph of the chip is presented with main blocks described. The Fig. 2 illustrates the architecture of a single recording channel. It consists of two amplifying stages AMP1 and AMP2 and an analogue multiplexer.

The input capacitor  $C_1$  separates the amplifier from the large DC offset generated on the electrode-tissue interface. The feedback of the front end amplifier is based on the  $C_2$



transistor. It allows to obtain very high resistances up to even  $10\text{ T}\Omega$  [12] which leads to very low cut-off frequency necessary in the Local Field Potential (LFP signals) measurements. The main disadvantages of such solutions are a strong dependence of the resistance value on the technology in which it was processed, limited control of such a resistance and large resistance spread from channel-to-channel which makes it difficult to obtain acceptable matching of the low cut-off frequencies in multichannel ASIC.

For this reason we used another solution, where a feedback resistance responsible for both setting the low cut-off frequency and biasing the input differential amplifier transistor is user dependent (see Fig. 2). The  $R_f$  resistance is built with the PMOS transistors combined as it is shown in the Fig. 4. Gate potentials of the feedback transistors MR1, MR2 are referenced either to the input or output of the AMP1 by the Level Shifters (LS). In order to control resistance of the MR1, MR2 transistors the  $V_{FOL}$  input is given. For the test purposes the  $I_{POL}$  input is provided to investigate the influence of the bulk polarization on the feedback MOS resistance. Both of them ( $V_{FOL}$ ,  $I_{POL}$ ) change the voltage shifting level of the LS circuits. The LS circuits are simple source followers with controlled gate-source voltage by the means of its current.

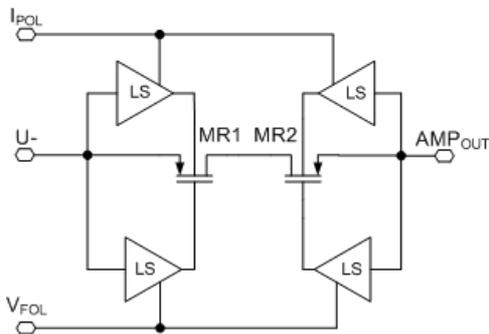


Fig. 4. Simplified scheme of the AMP1 resistive feedback.

### III. MEASUREMENT RESULTS

In order to perform tests of the described chip the 6 layer PCB board was designed equipped with the LVDS transmitters dedicated for chip communication. All measurements were performed using the NI-6259 measurement card and LabVIEW environment. Measurement results of the designed chip are presented below.

#### A. Pass-Band Settings

In the Fig. 5 the frequency responses for different channel settings are shown. Low cut-off frequency may be changed from 9 Hz up to 90 Hz thanks to the  $V_{FOL}$  input controlling the resistance of the AMP1 feedback. Next by changing the  $I_{BIAS}$  input in the range  $0.1\text{ V} \div 0.4\text{ V}$  the high cut-off frequency may be set in the  $1.6\text{ kHz} \div 24\text{ kHz}$  range.

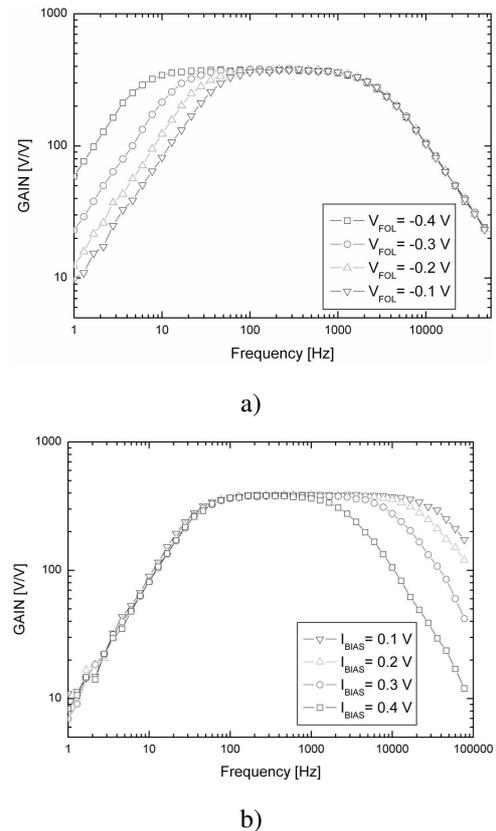


Fig. 5. Frequency response of single channel: a) low cut-off frequency tuning, b) high cut-off frequency tuning.

#### B. Channel-To-Channel Uniformity

In multichannel chip uniformity of analogue parameters from channel-to-channel (i.e. gain, cut-off frequencies) is the crucial aspect. In Fig. 6, 7, 8 the measured spread of a gain and cut-off frequencies are shown. These demonstrate that the spread of the gain is about 2% while the spread of the low and high cut-off frequencies are 10% and 4.5% respectively. The spread of the low cut-off frequency (which is higher than the other parameters) depends on the feedback capacitance and the effective feedback resistance. The effective feedback resistance is controlled by the level shifters which makes the overall spread of low cut-off frequency higher comparing to solution without such a control [13].

The Table I presents the spread of low cut-off frequency for different corner frequency settings. The spread decreases with increasing corner frequency, however in all cases it is within acceptable limit. Nevertheless this point of design is going to be improved in further version of this chip by using correction DAC's situated in the each recording channel independently.

TABLE I  
SPREAD OF LOW CUT-OFF FREQUENCY VS. ITS MEAN VALUE SETTING

Low cut-off frequency [Hz]	Spread of the low cut-off frequency [%]
9	22
20	16
36	10

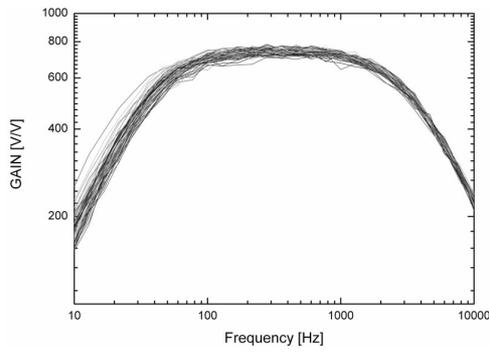


Fig. 6. Distribution of the gain for  $V_{FOL} = -0.2V$ .

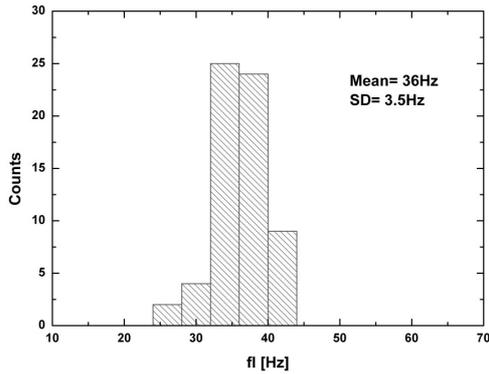


Fig. 7. Distribution of the low cut-off frequency for  $V_{FOL} = -0.2V$ .

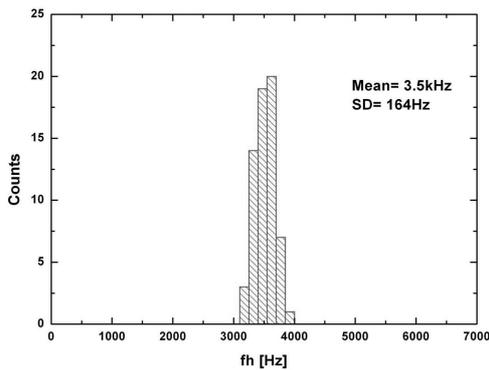


Fig. 8. Distribution of the high cut-off frequency for  $V_{FOL} = -0.2V$ .

### C. Noise Measurements

The Input Referred Noise (IRN) measurements were also taken. In order to show how the frequency band may influence the IRN the two opposing settings of the channel frequency band were employed:

- Setting I - frequency band: 9 Hz ÷ 24 kHz,
- Setting II - frequency band: 90 Hz ÷ 1.6 kHz.

Power spectral density measurements (see Fig. 9) show the frequency band impact on the overall channel noise. Also recorded channel output signals (see Fig. 10) show this relations.

Noise measurements show that for Setting I and Setting II input referred noise are equal  $9 \mu V$  and  $7 \mu V$  respectively



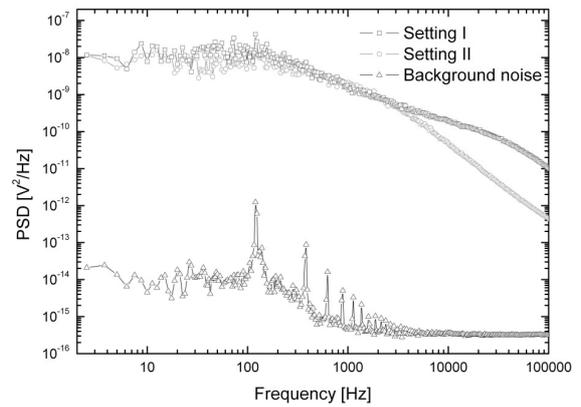


Fig. 9. Power spectral density of output noise of ASIC for two different pass-band settings and instrumentation noise.

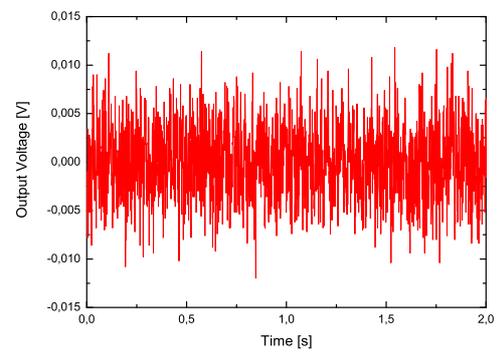

a)

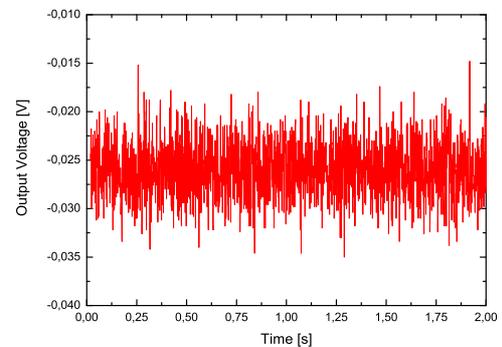

b)

Fig. 10. Typical output referred noise of the channel for different pass-band settings: a) Setting I, b) Setting II.

which are low enough for most in vivo and experiments.

### D. DC Coupling of the Consecutive Stages

So as to avoid propagation throughout the recording channel of the AMP1 DC offset the  $C_{AC}$  coupling capacitor

is used between AMP1 and AMP2 stages (see Fig. 2). The drawback of this solution is that it occupies additional area of the ASIC and introduces a very large time constants in the readout channel (because its corner frequency must be set to not suppress signals from single Hz band). These large time constants are crucial when the system is equipped with the stimulation circuits because the stimulation pulses may saturate input stages of the recording preamplifiers. As a result saturation of the AMP1 stage combined with the AC coupling circuits can increase the time between recording and stimulation phases. Thus we checked the DC spread of the channel output voltage with and without the AC coupling between the amplifying stages. The results (see Fig. 11) show that the channel work with the DC coupling is possible and its DC level spread is still acceptable by an external ADC converter.

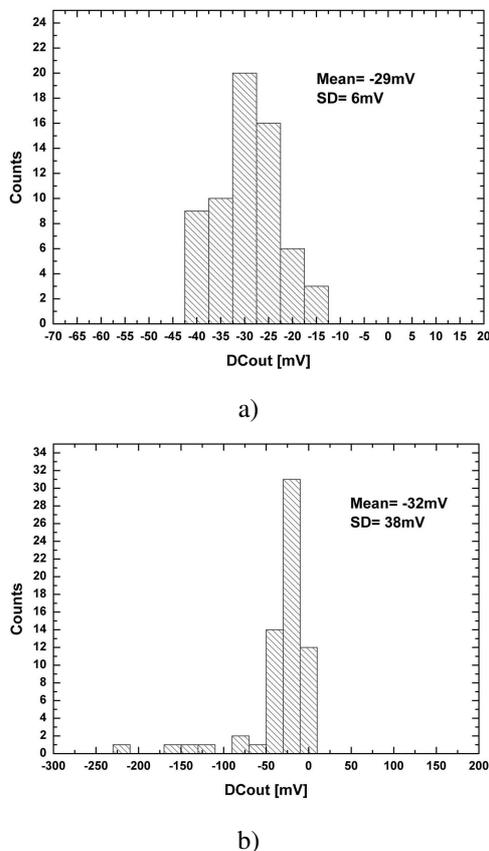


Fig. 11. Distribution of the output DC voltage for internal AC coupling: a) switched on, and b) switched off.

Nevertheless DC coupling of the recording channel may be limiting factor in systems where high channel gain is desirable. Thus we also checked whether it is possible to obtain high voltage gain of the recording channel while the DC coupling of the following stages is set. The Fig. 12 confirms that our 64 channels ASIC are capable to work properly with the DC coupling between amplifier stages and the channel-to-channel uniformity is preserved even in the case of the high gain setting.

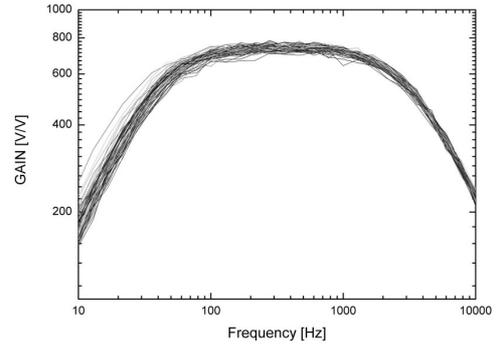


Fig. 12. Frequency response of the 64 channels for 700 V/V voltage gain with the DC coupling set.

### E. Systems with Multi-Electrode Arrays

We made an experiment using our prototype board and Multi-Electrode Array (MEA) provided by the Ayanda Biosystems. Into the saline solution in which MEA electrodes were immersed we dipped a metal round electrode with the signal conveyed from the generator. The recorded signals are depicted in the Fig. 13.

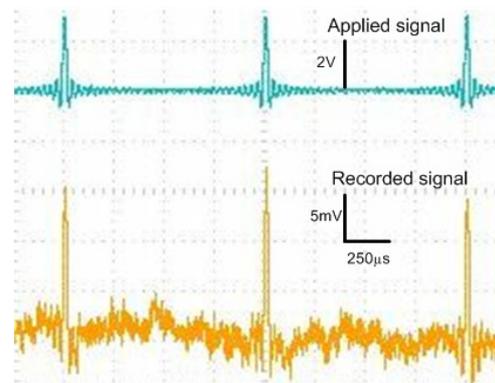


Fig. 13. Signals recorded with the MEA usage.

We have also designed a system for in vivo neurobiology experiments (see Fig. 14) which consists of the presented ASIC and 64 channel electrodes provided by the NEURONEXUS. Data acquisition will be made thanks to the PXI module (PCI eXtension for Instrumentation from National Instruments) equipped with the NI-PXI 6733 card and 100 MS/s, and 14-Bit Digitizer NI-PXI 5122. Overall system is controlled by the LabVIEW made application and will be used for measuring neural signals from the rat under anesthetic. We are going to start the neurobiology experiments soon.

## IV. SUMMARY

We presented the design and measurements of the 64 channel chip dedicated for neurobiology experiments. The

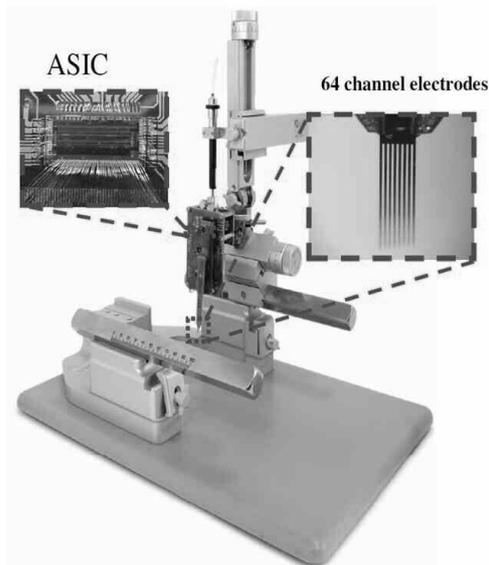


Fig. 14. 64 channel system for in vivo experiments.

ASIC is processed in 180 nm technology and its total area is about 13 mm<sup>2</sup>. Its essential parameters are summarized in Table II. The spread of the analogue parameters of the chip makes it suitable for building multichannel measurement system. The system has ability to control its gain and the cut-off frequencies which makes it useful to adapt into different neurobiology experiments.

TABLE II  
SUMMARY OF BASIC PARAMETERS OF ASIC

Parameter	Value
Gain	700 / 350 V/V
Tuning range for low cut-off frequency	9 ÷ 90 Hz
Tuning range for high cut-off frequency	1.6 ÷ 24 kHz
Equivalent input noise (depends on bandwidth setting)	7 ÷ 9 $\mu$ V
Power per channel	200 $\mu$ W
Power supply voltage	$\pm$ 0.9 V

#### ACKNOWLEDGMENT

The authors would like to thank Piotr Maj and Maciej Kachel (Department of Measurement and Instrumentation, AGH University of Science and Technology Krakow, Poland) for help during the tests of the chip.

#### REFERENCES

- [1] T. Jochum, T. Denison, and P. Wolf, "Integrated circuit amplifiers for multi-electrode intracortical recording," *Journal of Neural Engineering*, vol. 6, pp. 1–26, Jan. 2009.
- [2] S. K. Kelly and D. B. Shire, "Realization of a 15-channel, hermetically-encased wireless subretinal prosthesis for the blind," in *Proc. IEEE EMBC '09*, Minneapolis, USA, Sep. 2–6, 2009, pp. 200–203.
- [3] A. D. Dorval, N. Panjwani, R. Y. Qi, and W. M. Grill, "Deep brain stimulation that abolishes parkinsonian activity in basal ganglia improves thalamic relay fidelity in a computational circuit," in *Proc. IEEE EMBC '09*, Minneapolis, USA, Sep. 2–6, 2009, pp. 1565–1568.
- [4] R. R. Harrison, P. T. Watkins, R. J. Kier, R. O. Lovejoy, D. J. Black, B. Greger, and F. Solzbacher, "A low power integrated circuit for a wireless 100-electrode neural recording system," *IEEE J. Solid-State Circuits*, vol. 42, pp. 123–133, Jan. 2007.
- [5] R. F. Yazicioglu, P. Merken, R. Puers, and C. V. Hoof, "A 60 $\mu$ W 60nV sqrtHz readout front-end for portable biopotential acquisition systems," in *Proc. IEEE EMBC '09*, Minneapolis, USA, Sep. 2–6, 2009, pp. 200–203.
- [6] P. Kmon, M. Żołądź, P. Gryboś, and R. Szczygieł, "Design and measurements of 64-channel ASIC for neural signal recording," in *Proc. IEEE EMBC '09*, Minneapolis, USA, Sep. 2–6, 2009, pp. 528–531.
- [7] P. Gryboś, W. Dąbrowski, P. Hottowy, and T. Fiutowski, "Low noise multichannel front-end electronics for recording signals from alive neuronal cells," in *Proc. MIXDES 11th international conference*, Szczecin, Poland, Jun. 24–26, 2004, pp. 214–219.
- [8] A. Litke, N. Bezayiff, E. Chichilinsky, W. Cunningham, W. Dabrowski, A. Grillo, M. Grivich, P. Grybos, P. Hottowy, S. Kachiguine, R. Kalmar, K. Mathieson, D. Petrusca, M. Rahman, and A. Sher, "What does the eye tell the brain?: Development of system for the large-scale recording of retinal output activity," in *IEEE Nuclear Science Symposium*, Portland, USA, Oct. 19–25, 2003, pp. 951–955.
- [9] R. R. Harrison and C. Charles, "A low-power low-noise CMOS amplifier for neural recording applications," *IEEE J. Solid-State Circuits*, vol. 38, pp. 958–965, Jun. 2003.
- [10] M. Żołądź, P. Gryboś, M. Kachel, P. Kmon, and R. Szczygieł, "Analogue multiplexer for neural application in 180 nm CMOS technology," in *Proc. MIXDES 16th international conference*, Lodz, Poland, Jun. 25–27, 2009, pp. 230–233.
- [11] W. Wattanapanitch, M. Fee, and R. Sarpeshkar, "An energy-efficient micropower neural recording amplifier," *Transactions on Biomedical Circuits and Systems*, vol. 1, pp. 136–147, Jun. 2007.
- [12] M. Yin and M. Ghovanloo, "A low-noise preamplifier with adjustable gain and bandwidth for biopotential recording applications," in *IEEE International Symposium on Circuits and Systems, ISCAS 2007*, New Orleans, USA, May 27–30, 2007, pp. 321–324.
- [13] P. Kmon, P. Gryboś, R. Szczygieł, and M. Żołądź, "Multichannel system for in vivo and in vitro neural signal recording," *Electrical Review*, vol. 9, pp. 67–71, Sep. 2010.